

EtherCAT ACCESSORIES

TECHNICAL REFERENCE MANUAL

EtherCAT Accessories V25-2



2. About this document

This is the users manual for a series of EtherCAT Accessories available along with our devices.

2.1. Legend

The following symbols and formats will be used throughout the document.



Important

It gives you important information about the subject.
Please read carefully!



Hint

It gives you a hint or provides additional information about a subject.



Example

Gives you an example of a specific subject.

2.2. Online versions

2.2.1. Device Technical Reference Manual

The most recent version of this manual can be downloaded from our homepage:

<https://dewesoft.com/download/manuals>

In the *Hardware Manuals* section click the download link for the *Device® technical reference manual*.

2.2.2. DEWESoft® User Manual

The DEWESoft® User Manual document provides basics and additional information and examples for working with DEWESoft® and certain parts of the program.

The latest version of the DEWESoft® tutorials can be found here:

<https://dewesoft.com/download/manuals>

In the *Software Manuals* section click the download link of the DEWESoft X User Manual entry.

3. EtherCAT Accessories

EtherCAT stands for “Ethernet for Control Automation Technology.” It is a protocol that brings the power and flexibility of ethernet to the world of:


- industrial automation,
- motion control,
- real-time control systems, and
- data acquisition systems.



The EtherCAT protocol is maintained by the EtherCAT Technology Group and is **standardized under IEC 61158**.

Advantages of DAQ and EtherCAT

- High and low-speed data from advanced DAQ systems can now be integrated perfectly into a real-time control system
- Eliminating redundant A/D processing means less complexity, better accuracy, and real cost savings
- A separate very high-speed data file is available for advanced analysis if needed, and it is also synchronized with the PLC data

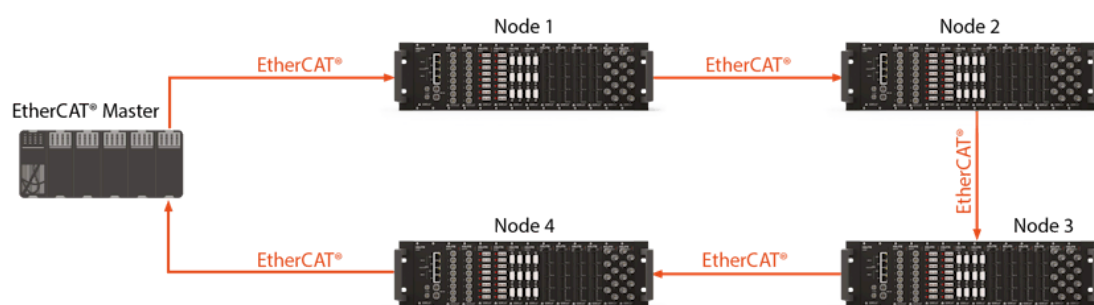

An example of EtherCAT network with ring topology



Channel expansion via additional EtherCAT equipped DAQ systems

3.1. ECAT Power Junction


The ECAT Power Junction box (article number: ECAT-POWER-JUNCTION) can be used to inject power into the Ethernet connection between your PC and the KRYPTON modules: so that you only have one cable for power and data to your KRYPTON modules.

Connector Label	Connector type	Info
POWER IN	2-pin LEMO male	9 - 48 VDC: e.g. for connection from the Power-Out connector of a Sirius slice
Ethernet	RJ-45	Ethernet data connection to your PC The Ethernet cable should always be shielded! You can use an EIA568-B straight or crossover cable.
EtherCAT	8-pin LEMO female	Power and Data connection to your KRYPTON module/s use any of the ECAT to ECAT expansion cables (e.g. LIT8m-LIT8f-10M)



ECAT Power junction

3.1.1. Power in connector: Pinout

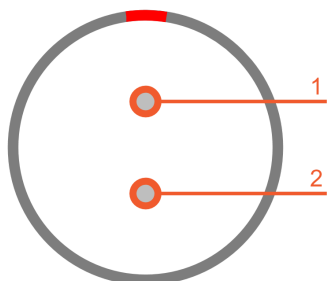

Pin	Name	Description
1	IN+	Input +
2	IN-	Input -

Power junction connector: pinout (2-pin LEMO male)

POWER IN connector (on the device): EXJ.1B.302.HLD

Mating connector (for the cable): FGJ.1B.302.CLLD

Power will be connected from 2-pin PS LEMO V+ to VCC of the 8-pin LEMO. V- is GND on the 8-pin LEMO.


3.1.2. RJ45 connector: Pinout



Ethernet connector: pinout (RJ-45 female)

Pin	Name	Description
1	TX_P	Transmission +
2	TX_N	Transmission -
3	RX_P	Reception +
4	-	-
5	-	-
6	RX_N	Reception -
7	-	-
8	-	-

3.1.3. EtherCAT connector: Pinout

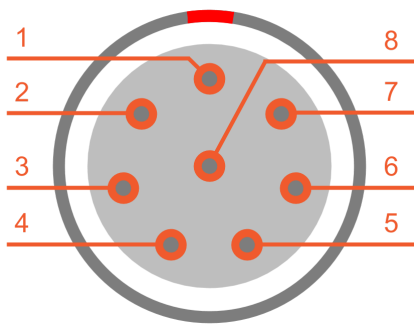

ECAT connector: pinout (8-pin LEMO female)


Pin	Name	Description
1	TX_P	Transmission +
2	TX_N	Transmission -
3	RX_P	Reception +
4	RX_N	Reception -
5	VCC	PWR IN
6	VCC	PWR IN
7	GND	Ground
8	GND	Ground

IN connector (on the device): EGG.IT.308.CLN
Mating connector (for the cable): FGG.IT.308.CLAC65Z

3.2. ECAT Power Injector

The ECAT Power Injector box (article number: ECAT Power Injector) can be used to inject power into the Ethernet connection between KRYPTON modules, when you can have a very long measurement chain.

Connector Label	Connector type	Info
PWR	8-pin LEMO female	Max. 48 VDC
↓ EtherCAT In ↑ EtherCAT Out	8-pin LEMO	Power and Data connection to your KRYPTON module/s use any of the ECAT to ECAT expansion cables (e.g. LIT8m-LIT8f-10M)
GND	Banana	Ground connection

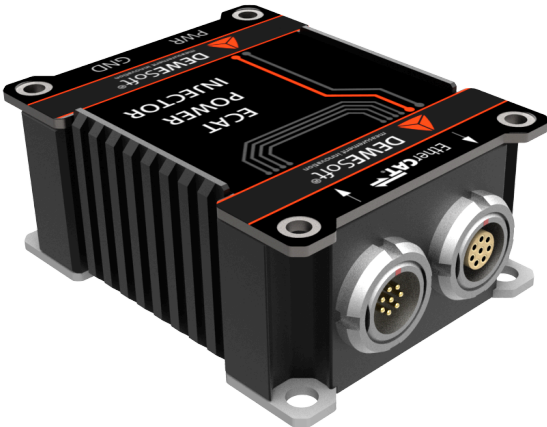


ECAT Power injector

3.2.1. ECAT Power Injector: Specifications

EtherCAT POWER INJECTOR	
Interface	
Data interface	EtherCAT®
Data Rate	100 Mbps Full Duplex bus speed
Max. Throughput per Chain	From 6 MB/s to 10 MB/s (see 1)
Sync Accuracy	< 200 ns within same EtherCAT chain < 2 µs using sync for multiple EtherCAT chains below 1 sample to Sirius®
EtherCAT®	Max. Cable Length 100 m
Max. Number of Units	64 or more (power injectors may be required)
Data Interface Connection	LEMO 1T EtherCAT® hybrid cable Single cable for data, power and sync, daisy chainable
Power specification	
Power Supply	9-48 V DC (see 2)
Environmental specification	
Operating Temperature	-40 to 85°C
Storage Temperature	-40 to 85°C
IP rating	IP67
1) It depends on the devices connected, numbers of channels, configuration, length of cables and other parameters.	
2) Passes through the EtherCAT signal, but cuts the power lines on the input.	

3.2.2. PWR connector: Pinout

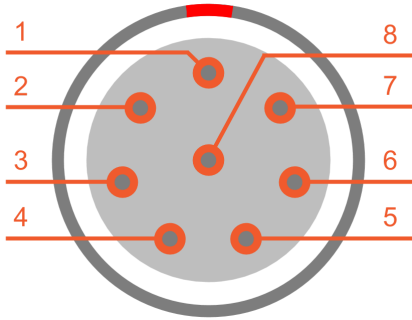


PWR connector: pinout (8-pin LEMO female)

Pin	Name	Description
1	-	-
2	-	-
3	-	-
4	-	-
5	VCC	PWR OUT
6	VCC	PWR OUT
7	GND	Ground
8	GND	Ground

IN connector (on the device): EGG.1T.308.CLN

Mating connector (for the cable): FGG.1T.308.CLA.1433

3.2.3. EtherCAT OUT connector: Pinout

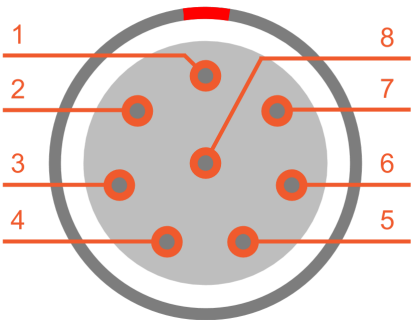

ECAT connector: pinout (8-pin LEMO female)


Pin	Name	Description
1	TX_P	Transmission +
2	TX_N	Transmission -
3	RX_P	Reception +
4	RX_N	Reception -
5	VCC	PWR IN
6	VCC	PWR IN
7	GND	Ground
8	GND	Ground

IN connector (on the device): EGG.1T.308.CLN

Mating connector (for the cable): FGG.1T.308.CLA.1433

3.2.4. EtherCAT IN connector: Pinout

The connector for EtherCAT is a LEMO 1T 8-pin male connector.

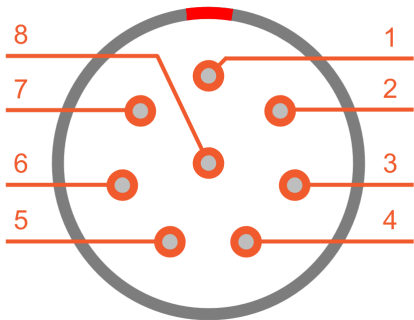

IN connector: pinout (8-pin LEMO male)

Pin	Name	Description
1	TX_P	Transmission +
2	TX_N	Transmission -
3	RX_P	Reception +
4	RX_N	Reception -
5	-	-
6	-	-
7	-	-
8	-	-

IN connector (on the device): EGJ.1T.308.CLD
Mating connector (for the cable): FGJ.1T.308.CLL.1433

3.3. ECAT Sync Junction

The ECAT Sync Junction box can be used to inject the sync signal into the EtherCAT line. The source of the sync signal must be IRIG B DC: thus, the sync signal of Sirius USB slices can be directly connected to the ECAT Sync Junction box.

Connector Label	Connector type	Info
IN	8-pin LEMO	EtherCAT input connector: e.g. connection to the PC via LIT8f-RJ45-1M cable
OUT	8-pin LEMO	EtherCAT output connector to your KRYPTON slice/s use any of the ECAT to ECAT expansion cables (e.g. LIT8m-LIT8f-10M).
SYNC	4-pin LEMO	Input connector for the IRIG-B-DC signal (TTL level), e.g. external, or directly from Sirius USB Note: the two SYNC connectors are directly connected, so you can use the other connector as output (to daisy-chain the same sync signal to other devices: e.g. DEWE-43-A, DS-CAM, etc.)




ECAT sync junction

3.3.1. ECAT Sync Junction: Specifications

Interface	
Data interface	EtherCAT®
Data Rate	100 Mbps Full Duplex bus speed
Max. Throughput per Chain	From 6 MB/s to 10 MB/s (see 1)
Sync Accuracy	< 200 ns within same EtherCAT chain < 2 µs using sync for multiple EtherCAT chains below 1 sample to Sirius®
EtherCAT®	Max. Cable Length 100 m
Max. Number of Units	64 or more (power injectors may be required)
Data Interface Connection	LEMO 1T EtherCAT® hybrid cable Single cable for data, power and sync, daisy chainable
Power specification	
Power Supply	9-48 V DC
Current	8 A DC max
Power Consumption	Typ. 1.3 W (Max. 1.5 W) (without additional power daisy-chain)

Environmental specification	
Operating Temperature	-40 to 70°C
Storage Temperature	-40 to 85°C
Shock & Vibration	Shock: SIST EN 60068-2-27:2009 (100 g, 6 ms) Random vibration
1) It depends on the devices connected, numbers of channels, configuration, length of cables and other parameters.	

3.3.2. EtherCAT out connector: Pinout

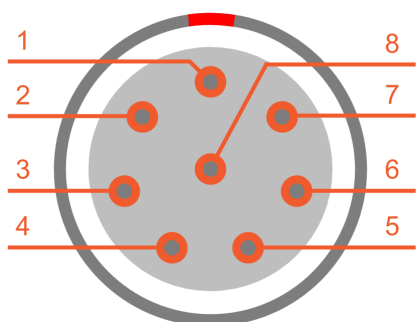


OUT connector: pinout (8-pin LEMO female)

IN connector (on the device): EGG.1T.308.CLN
Mating connector (for the cable):
FEG.1T.308.CLA.1433

Pin	Name	Description
1	TX_P	Transmission +
2	TX_N	Transmission -
3	RX_P	Reception +
4	RX_N	Reception -
5	VCC	PWR IN
6	VCC	PWR IN
7	GND	Ground
8	GND	Ground

3.3.3. EtherCAT in connector: Pinout

The connector for EtherCAT is a LEMO 1T 8-pin male connector.

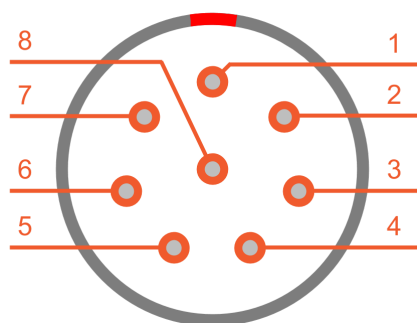

IN connector: pinout (8-pin LEMO male)


IN connector (on the device): EGJ.1T.308.CLD

Pin	Name	Description
1	TX_P	Transmission +
2	TX_N	Transmission -
3	RX_P	Reception +
4	RX_N	Reception -
5	VCC	PWR IN
6	VCC	PWR IN
7	GND	Ground

Mating connector (for the cable):
FGJ.1T.308.CLL.1433

8	GND	Ground
---	-----	--------

3.3.4. Sync connector: Pinout

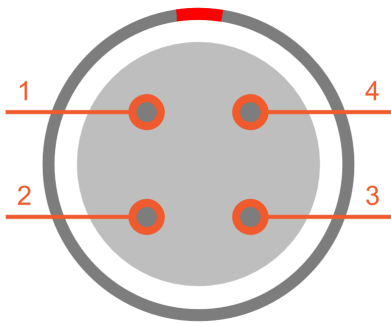

Sync connector: pinout (4-pin LEMO female)

Pin	Name	Description
1	CLK	Clock
2	Trigg	Trigger
3	GPS-PPS	GPS - PPS
4	DGND	Digital Ground

Interface connector: EEG.00.304.CLL
Mating connector: FGG.00.304.CLAD27Z

3.5. ECAT Repeater

The EtherCAT Repeater is a part of EtherCAT accessories used for the extension of EtherCAT hybrid cables allowing maximum connection of two 50 meters long cables. It increases connection stability for distributed EtherCAT systems with distances between measurement units larger than 50 meters.

EtherCAT Repeater is a rugged inline device with an IP67 rating and corresponds to MIL-STD-810D standard. It has a LEMO IT Series 8-pin male connector on the IN port and a female connector on the OUT port. Pinout corresponds to the standard KRYPTON devices.




EtherCAT Repeater

3.5.1. EtherCAT Repeater: Specifications

Interface	
Data interface	EtherCAT®
Data Rate	100 Mbps Full Duplex bus speed
Max. Throughput per Chain	From 6 MB/s to 10 MB/s (see 1)
Sync Accuracy	below 1 sample to Sirius®
EtherCAT®	Max. Cable Length 50 m
Data Interface Connection	LEMO 1T EtherCAT® hybrid cable Single cable for data, power and sync, daisy chainable
Input connector	LIT8m (data, power and sync)
Output connector	LIT8f (data, power and sync)
Power	
Power supply	9 - 48 VDC
Maximum current	max. 7.5 A
Power consumption	Typ. 0.72 W, Max. 1 W
Environmental	
Operating Temperature	-40 to 85 °C
Storage Temperature	-40 to 85 °C
Humidity	5 to 95 % RH non-condensing at 50 °C
IP rating	IP67
Shock & Vibration	Vibration sweep sinus (EN 60068-2-6:2008) Vibration random (EN 60721-3-2: 1997 - Class 2M2) Shock (EN 60068-2-27:2009) MIL-STD-810D
Physical	
Dimensions	85.3 x 35 x 34 mm (incl. connectors)
Weight	190 g
1) It depends on the devices connected, numbers of channels, configuration, length of cables and other parameters.	

3.5.2. EtherCAT out connector: Pinout

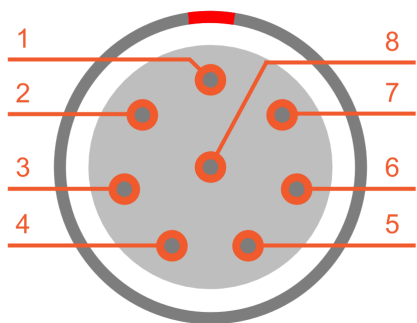

OUT connector: pinout (8-pin LEMO female)


Pin	Name	Description
1	TX_P	Transmission +
2	TX_N	Transmission -
3	RX_P	Reception +
4	RX_N	Reception -
5	VCC	PWR IN
6	VCC	PWR IN
7	GND	Ground
8	GND	Ground

IN connector (on the device): EGG.1T.308.CLN

Mating connector (for the cable): FGG.1T.308.CLA.1433

3.5.3. EtherCAT in connector: Pinout

The connector for EtherCAT is a LEMO 1TB 8-pin male connector.

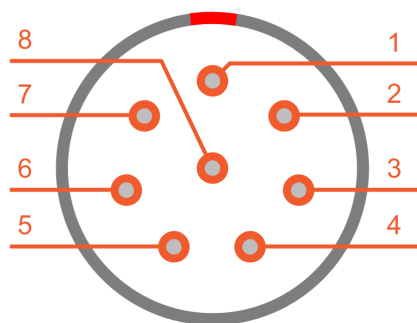

IN connector: pinout (8-pin LEMO male)

Pin	Name	Description
1	TX_P	Transmission +
2	TX_N	Transmission -
3	RX_P	Reception +
4	RX_N	Reception -
5	VCC	PWR IN
6	VCC	PWR IN
7	GND	Ground
8	GND	Ground

IN connector (on the device): EGJ.1T.308.CLD

Mating connector (for the cable): FGJ.1T.308.CLL.1433

4. Warranty information

Notice

The information contained in this document is subject to change without notice.

Note:

Dewesoft d.o.o. shall not be liable for any errors contained in this document. Dewesoft MAKES NO WARRANTIES OF ANY KIND WITH REGARD TO THIS DOCUMENT, WHETHER EXPRESS OR IMPLIED. DEWESOFT SPECIFICALLY DISCLAIMS THE IMPLIED WARRANTIES OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE. Dewesoft shall not be liable for any direct, indirect, special, incidental, or consequential damages, whether based on contract, tort, or any other legal theory, in connection with the furnishing of this document or the use of the information in this document.

The copy of the specific warranty terms applicable to your Dewesoft product and replacement parts can be obtained from your local sales and service office. To find a local dealer for your country, please visit <https://dewesoft.com/support/distributors>.

4.1. Calibration

Every instrument needs to be calibrated at regular intervals. The standard norm across nearly every industry is annual calibration. Before your Dewesoft data acquisition system is delivered, it is calibrated. Detailed calibration reports for your Dewesoft system can be requested. We retain them for at least one year, after system delivery.

4.2. Support

Dewesoft has a team of people ready to assist you if you have any questions or any technical difficulties regarding the system. For any support please contact your local distributor first or Dewesoft directly.

Dewesoft d.o.o.
Gabrsko 11a
1420 Trbovlje Slovenia

Europe Tel.: +386 356 25 300
Web: <http://www.dewesoft.com>
Email: Support@dewesoft.com
The telephone hotline is available Monday to Friday from 07:00 to 16:00 CET (GMT +1:00)

4.3. Service/repair

The team of Dewesoft also performs any kinds of repairs to your system to assure a safe and proper operation in the future. For information regarding service and repairs please contact your local distributor first or Dewesoft directly on <https://dewesoft.com/support/rma-service>.

4.4. Restricted Rights

Use Slovenian law for duplication or disclosure. Dewesoft d.o.o. Gabrsko 11a, 1420 Trbovlje, Slovenia / Europe.

4.5. Copyright

Copyright © 2015-2026 Dewesoft d.o.o. This document contains information which is protected by copyright. All rights are reserved. Reproduction, adaptation, or translation without prior written permission is prohibited, except as allowed under the copyright laws. All trademarks and registered trademarks are acknowledged to be the property of their owners.

4.6. Trademarks

We take pride in our products and we take care that all key products and technologies are registered as trademarks all over the world. The Dewesoft name is a registered trademark. Product families (KRYPTON, SIRIUS, DSI, DS-NET) and technologies (DualCoreADC, SuperCounter, GrandView) are registered trademarks as well. When used as the logo or as part of any graphic material, the registered trademark sign is used as a part of the logo. When used in text representing the company, product or technology name, the ® sign is not used. The Dewesoft triangle logo is a registered trademark but the ® sign is not used in the visual representation of the triangle logo.

5. Safety instructions

Your safety is our primary concern! Please be safe!

5.1. Safety symbols in the manual

Safety reference manual for the IOLITE Data Acquisition Devices can be found in <https://dewesoft.com/download> section. Search for keyword: **Safety technical reference manual**



Warning

Calls attention to a procedure, practice, or condition that could cause the body injury or death



Caution

Calls attention to a procedure, practice, or condition that could possibly cause damage to equipment or permanent loss of data.

5.2. General Safety Instructions



Warning

The following general safety precautions must be observed during all phases of operation, service, and repair of this product. Failure to comply with these precautions or with specific warnings elsewhere in this manual violates safety standards of design, manufacture, and intended use of the product. Dewesoft d.o.o. assumes no liability for the customer's failure to comply with these requirements.

All accessories shown in this document are available as an option and will not be shipped as standard parts.

5.2.1. Environmental Considerations

The product is an electronic instrument designed with consideration for environmental impact during its design and use phase. The materials and components used comply with the requirements of the RoHS Directive (2011/65/EU) and the REACH Regulation (EC No. 1907/2006), with no intentional use of restricted or prohibited hazardous substances. During normal operation, the product does not generate direct environmental emissions and features low power consumption. The device is designed for long-term use and serviceability, supporting an extended product lifetime. The product enclosure is made of aluminum, and selected components of the product are suitable for material recycling.

5.2.2. Product End-of-Life Handling

At the end of its service life, the product shall not be disposed of as unsorted municipal waste and shall be collected separately in accordance with the WEEE Directive (2012/19/EU).



The crossed-out wheeled bin symbol on the product, packaging, or accompanying documentation indicates that the equipment must be returned to an authorized collection point for waste electrical and electronic equipment. Recycling, recovery, and disposal activities shall be carried out by authorized operators in compliance with applicable local, national, and EU environmental regulations.

For proper treatment, recovery and recycling of old products and batteries, please take them to applicable collection points in accordance with your national legislation. Penalties may be applicable for incorrect disposal of this waste, in accordance with national legislation.

5.2.3. General safety and hazard warnings for all Dewesoft systems

Safety of the operator and the unit depend on following these rules.

- Use this system under the terms of the specifications only to avoid any possible danger.
- Read your manual before operating the system.
- Observe local laws when using the instrument.
- DO NOT touch internal wiring!
- DO NOT use higher supply voltage than specified!
- Use only original plugs and cables for harnessing.
- You may not connect higher voltages than rated to any connectors.
- The power cable and connector serve as Power-Breaker. The cable must not exceed 3 meters, the disconnect function must be possible without tools.
- Maintenance must be executed by qualified staff only.
- During the use of the system, it might be possible to access other parts of a more comprehensive system. Please read and follow the safety instructions provided in the manuals of all other components regarding warning and security advice for using the system.
- With this product, only use the power cable delivered or defined for the host country.
- DO NOT connect or disconnect sensors, probes or test leads, as these parts are connected to a voltage supply unit.
- Ground the equipment: For Safety Class 1 equipment (equipment having a protective earth terminal), a non-interruptible safety earth ground must be provided from the mains power source to the product input wiring terminals.

- Please note the characteristics and indicators on the system to avoid fire or electric shocks. Before connecting the system, please read the corresponding specifications in the product manual carefully.
- The inputs must not, unless otherwise noted (CATx identification), be connected to the main circuit of category II, III and IV.
- The power cord separates the system from the power supply. Do not block the power cord, since it has to be accessible for the users.
- DO NOT use the system if equipment covers or shields are removed.
- If you assume the system is damaged, get it examined by authorized personnel only.
- Adverse environmental conditions are Moisture or high humidity Dust, flammable gases, fumes or dissolver Thunderstorm or thunderstorm conditions (except assembly PNA) Electrostatic fields, etc.
- The measurement category can be adjusted depending on module configuration.
- Any other use than described above may damage your system and is attended with dangers like short-circuiting, fire or electric shocks.
- The whole system must not be changed, rebuilt or opened.
- DO NOT operate damaged equipment: Whenever it is possible that the safety protection features built into this product have been impaired, either through physical damage, excessive moisture, or any other reason, REMOVE POWER and do not use the product until the safe operation can be verified by service-trained personnel. If necessary, return the product to Dewesoft sales and service office for service and repair to ensure that safety features are maintained.
- If you assume a more riskless use is not provided anymore, the system has to be rendered inoperative and should be protected against inadvertent operation. It is assumed that a more riskless operation is not possible anymore if the system is damaged obviously or causes strange noises. The system does not work anymore. The system has been exposed to long storage in adverse environments. The system has been exposed to heavy shipment strain.
- Warranty void if damages caused by disregarding this manual. For consequential damages, NO liability will be assumed!
- Warranty void if damage to property or persons caused by improper use or disregarding the safety instructions.
- Unauthorized changing or rebuilding the system is prohibited due to safety and permission reasons (CE).
- Be careful with voltages >25 VAC or >35 VDC! These voltages are already high enough in order to get a perilous electric shock by touching the wiring.
- The product heats during operation. Make sure there is adequate ventilation. Ventilation slots must not be covered!
- Only fuses of the specified type and nominal current may be used. The use of patched fuses is prohibited.
- Prevent using metal bare wires! Risk of short circuit and fire hazard!
- DO NOT use the system before, during or shortly after a thunderstorm (risk of lightning and high energy over-voltage). An advanced range of application under certain conditions is allowed with therefore designed products only. For details please refer to the specifications.
- Make sure that your hands, shoes, clothes, the floor, the system or measuring leads, integrated circuits and so on, are dry.
- DO NOT use the system in rooms with flammable gases, fumes or dust or in adverse environmental conditions.
- Avoid operation in the immediate vicinity of high magnetic or electromagnetic fields, transmitting antennas or high-frequency generators, for exact values please refer to enclosed specifications.

- Use measurement leads or measurement accessories aligned with the specification of the system only. Fire hazard in case of overload!
- Lithium ion batteries are classified as not hazardous when used according to the recommendations of the manufacturer described in Battery Safety Data Sheet, which is available for download from [this link](#).
- Do not switch on the system after transporting it from a cold into a warm room and vice versa. The thereby created condensation may damage your system. Acclimatise the system unpowered to room temperature.
- Do not disassemble the system! There is a high risk of getting a perilous electric shock. Capacitors still might be charged, even if the system has been removed from the power supply.
- The electrical installations and equipment in industrial facilities must be observed by the security regulations and insurance institutions.
- The use of the measuring system in schools and other training facilities must be observed by skilled personnel.
- The measuring systems are not designed for use in humans and animals.
- Please contact a professional if you have doubts about the method of operation, safety or the connection of the system.
- Please be careful with the product. Shocks, hits and dropping it from already- lower level may damage your system.
- Please also consider the detailed technical reference manual as well as the security advice of the connected systems.
- This product has left the factory in safety-related flawlessness and in proper condition. In order to maintain this condition and guarantee safety use, the user has to consider the security advice and warnings in this manual.

EN 61326-3-1:2008

IEC 61326-1 applies to this part of IEC 61326 but is limited to systems and equipment for industrial applications intended to perform safety functions as defined in IEC 61508 with SIL 1-3.

The electromagnetic environments encompassed by this product family standard are industrial, both indoor and outdoor, as described for industrial locations in IEC 61000-6-2 or defined in 3.7 of IEC 61326-1.

Equipment and systems intended for use in other electromagnetic environments, for example, in the process industry or in environments with potentially explosive atmospheres, are excluded from the scope of this product family standard, IEC 61326-3-1.

Devices and systems according to IEC 61508 or IEC 61511 which are considered as “operationally well-tried”, are excluded from the scope of IEC 61326-3-1.

Fire-alarm and safety-alarm systems, intended for the protection of buildings, are excluded from the scope of IEC 61326-3-1.

5.3. Documentation version history

Version	Date	Notes
V23-1	2.10.2023	- Initial version, a collection of information from multiple manuals
V25-1	27.3.2025	- Added specifications for Ethercat Power Injector - Deleted the bandwidth limitation for DS-HUBe7
V25-2	21.7.2025	- Corrected the input voltage for GPS CLOCK - Corrected IOLITE power junction and IOLITE repeater